


# Certificate of Analysis

## Reference Material & Standard

|                    |                        |                   |                                                                                     |
|--------------------|------------------------|-------------------|-------------------------------------------------------------------------------------|
| Product Name:      | 1,2-Dichlorobenzene D4 | Catalogue Number: | CCEM500036                                                                          |
| Synonyms:          | N/A                    | Lot Number:       | 0824-RC-0084                                                                        |
| CAS Number:        | 2199-69-1              | Expiry Date:      | Apr 23, 2029                                                                        |
| Molecular Formula: | C6D4Cl2                | Storage:          | 2°C ~ 8°C Protected from light and Sealed                                           |
| Molecular Weight:  | 151.03                 | Warning:          |  |

Chemical Structure:

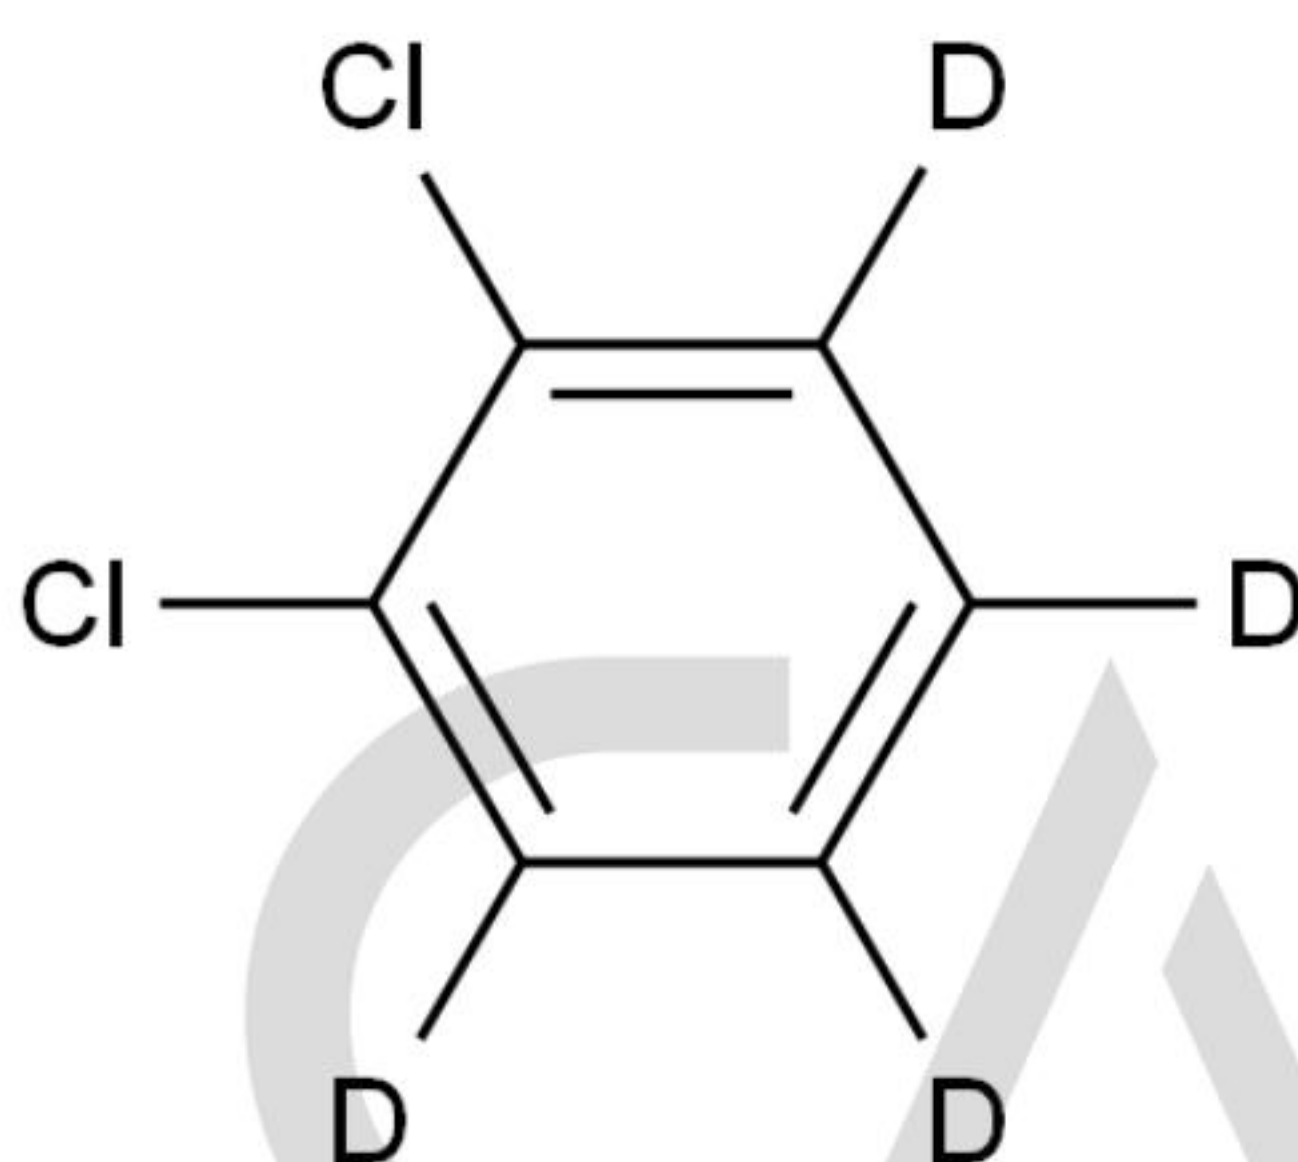

| Test Items      | Method            | Results           |
|-----------------|-------------------|-------------------|
| Appearance      | Visual inspection | Colourless Liquid |
| Identification  | GCMS&CNMR         | Confirmed         |
| Chemical Purity | GC                | 100.000%          |
| Isotopic Purity |                   | 99.5%             |
| Water Content   | Karl Fischer      | 0.1753%           |
| Assay           |                   | 99.8%             |
| Uncertainty     |                   | ±0.2%             |

## Comment:

1. The calculation of the 100% method follows the formula (calculated on the non-dried basis):

$$\text{Assay (\%)} = (100\% - \text{Water Content}) * \text{Purity GC (\%)} / 100\%$$

Water Content is considered as absolute effect, GC purity is considered as relative effect.

2. The uncertainty values are the expanded uncertainty and represent an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

## Signature:

Prepared by:

*Lisa*

Reviewed by:

*Hinlam*

Approved by General Manager:

*David*

Date: May 14, 2025

Date: May 14, 2025

Date: May 14, 2025

